

### WHICH FILE FOR WHICH CASE?

#### TREATMENT







##### STANDARD CASES

##### DIFFICULT CASES

CONTINUOUS ROTATION

ALTERNATING  
Anti-clockwise and clockwise movement

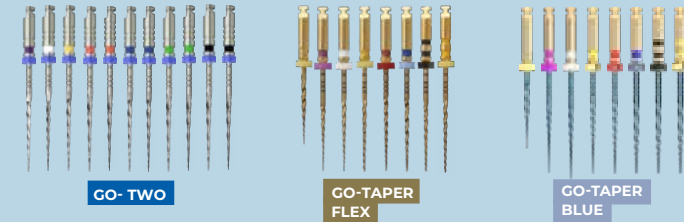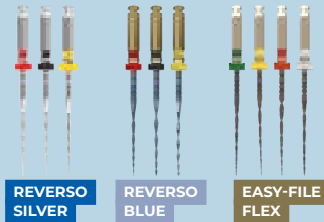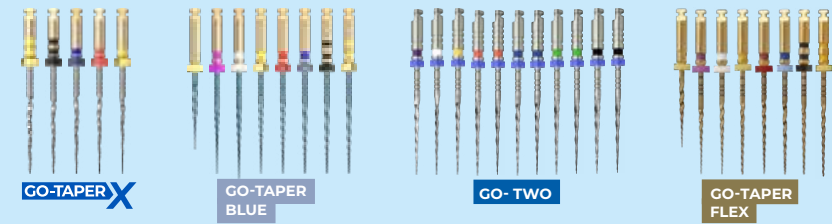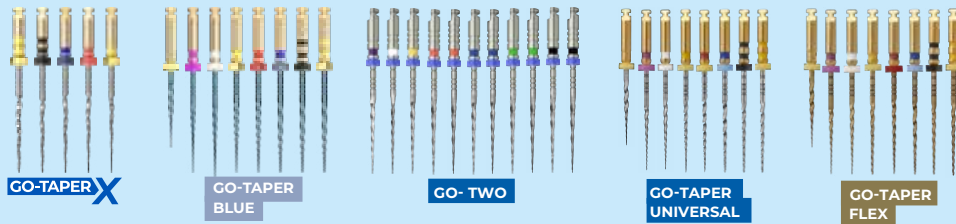

#### PRE-ENLARGEMENT


#### RETREATMENT


CONTINUOUS ROTATION

ALTERNATING  
Anti-clockwise and clockwise movement

CONTINUOUS ROTATION

ALTERNATING  
Anti-clockwise and clockwise movement

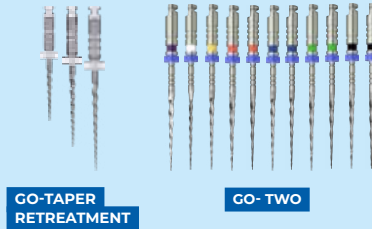




Flexibility



Cutting Power



Resistance



Already Sterile

Straight and/or relatively wide canals - Narrow and/or curved canals

**WHICH FILE FOR WHICH USE?**

**FOR a quick and reliable canal preparation,  
WITH a clear and precise protocol**

**ORIFICE OPENER**

GO-TAPER BLUE A0

GO-TAPER FLEX A0

GO-TAPER UNIVERSAL A0

**CATHETERISM**

PREFILE

**PRE-ENLARGEMENT**

GO GLIDER

EASY-FILE FLEX GLIDER

**CANAL SHAPING**

GO-TAPER UNIVERSAL

GO-TAPER FLEX

EASY-FILE FLEX

GO-TAPER X

GO-TAPER BLUE

REVERSO BLUE

GO-TWO

REVERSO SILVER

**ROOT CANAL RETREATMENT**

GO-TWO

GO-TAPER RETREATMENT

REVERSO SILVER

Class IIa medical devices.

GO-TAPER FLEX, PREFILE, EASY-FILE FLEX GLIDER : CE 0197 mark. Notified body TÜV Rheinland. European representative : SUNGO Europe B.B. Olympisch Stadion 24, 1076DE Amsterdam, The Netherlands. GO-TAPER UNIVERSAL, GO-TWO, GO-TAPER RETREATMENT, REVERSO SILVER, REVERSO, BLUE, EASY-FILE FLEX, GO-TAPER BLUE, GO-TAPER X, GO GLIDER. CE 0425 mark. Notified body ICIM. Fabricant: CFPM 2 bis chemin du Loup, 93290, Tremblay-en-France, FRANCE.